


FilmArray Blood Culture Identification Panel

1 Test. 27 Targets. All in about an hour.



Gram-Positive Bacteria

Enterococcus
Listeria monocytogenes
Staphylococcus
Staphylococcus aureus
Streptococcus
Streptococcus agalactiae
Streptococcus pyogenes
Streptococcus pneumoniae




Gram-Negative Bacteria

Acinetobacter baumannii
Haemophilus influenzae
Neisseria meningitidis
Pseudomonas aeruginosa
Enterobacteriaceae
Enterobacter cloacae complex
Escherichia coli
Klebsiella oxytoca
Klebsiella pneumoniae
Proteus
Serratia marcescens




Yeast

Candida albicans
Candida glabrata
Candida krusei
Candida parapsilosis
Candida tropicalis



Antibiotic Resistance Genes

mecA - methicillin resistant
vanA/B - vancomycin resistant
KPC - carbapenem resistant

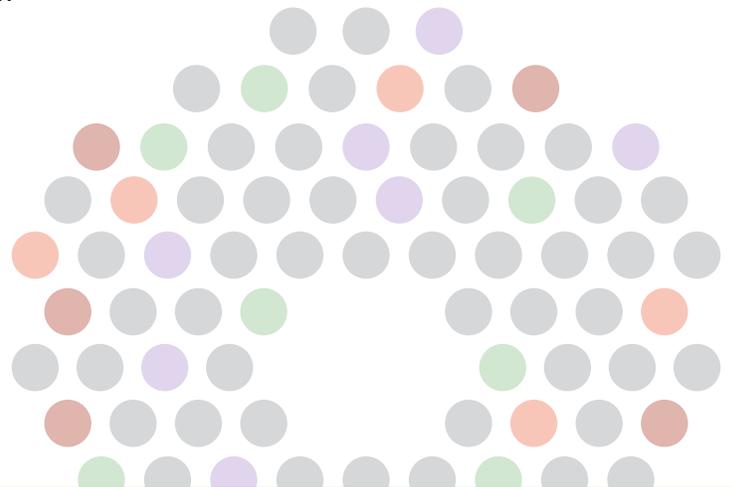

1
Hour

Identify Pathogens from Positive Blood Cultures in About 1 Hour

For In-vitro Diagnostic Use
FDA Cleared | CE IVD Marked

The FilmArray Blood Culture Identification Panel (BCID) tests for a comprehensive list of 24 pathogens and 3 antibiotic resistance genes associated with bloodstream infections. With just one test you can identify pathogens in 9 out of 10 positive blood cultures in about an hour with only 2 minutes of hands-on time.

- **Simple:** 2 minutes of hands-on time
- **Easy:** No precise measuring or pipetting required
- **Fast:** Turnaround time of about 1 hour
- **Comprehensive:** 27 target BCID panel



If you are interested in a free, no obligation demonstration of the FilmArray in your laboratory visit www.biofiredx.com or call 1-800-735-6544.

FREE Demo!



Panel Specifications

Sample Handling	Performance Parameters
<ul style="list-style-type: none"> Sample Type: Positive Blood Culture Sample Volume: 200 µL 	<ul style="list-style-type: none"> Hands-on time: 2 minutes Run turnaround time: about 1 hour


How Does the FilmArray Work?

The FilmArray reagent pouch stores all the necessary reagents for sample preparation, PCR and detection in a freeze-dried format. Prior to a run, the user injects Hydration Solution and positive blood culture sample combined with Sample Buffer into the pouch. The FilmArray instrument does the rest.


First, the FilmArray extracts and purifies all nucleic acids from the sample. Next, the FilmArray performs a nested multiplex PCR. During the first-stage PCR, the FilmArray performs a single, large volume, massively multiplexed reaction. Last, individual singleplex second-stage PCR reactions detect the products from the first stage PCR.

Using endpoint melting curve data, the FilmArray software automatically generates a result for each target in a single report.

Setting up the FilmArray is Easy – Sample in, Results out

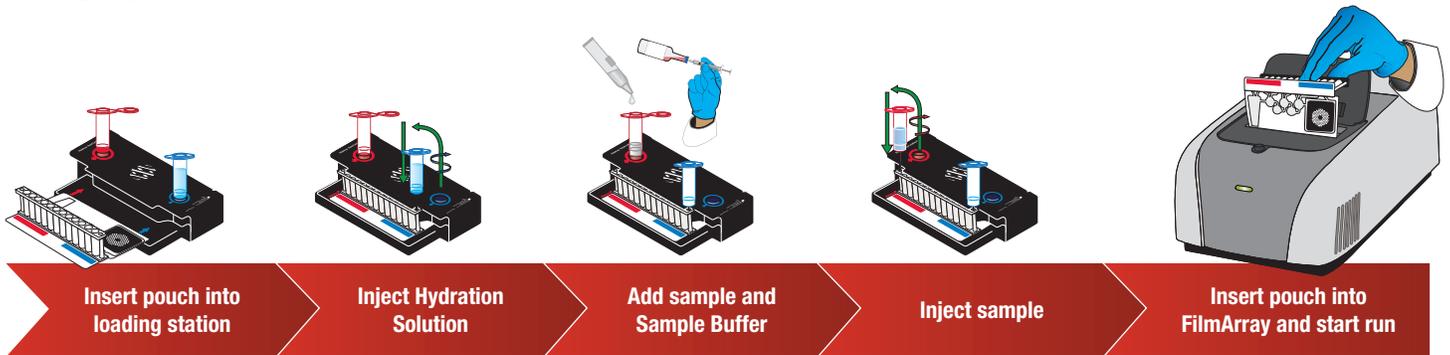

The FilmArray Pouch and Analysis Report

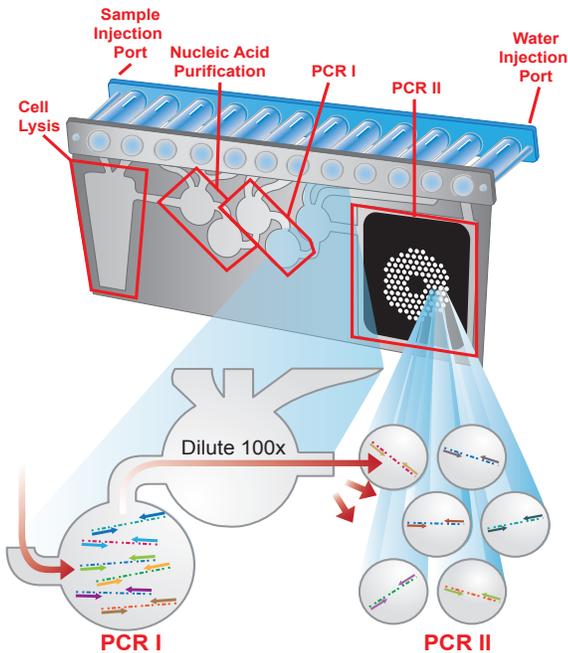

FilmArray® BCID Panel		BIOFIRE www.BioFireDx.com	
Run Summary			
Sample ID:	SDY_9621_LED_50_6	Run Date:	29 May 2013 3:41 PM
Organisms Detected:	<i>Enterobacteriaceae</i> <i>Klebsiella pneumoniae</i>	Controls:	Passed
Applicable Antimicrobial Resistance Genes:	KPC - Detected		
Result Summary - Interpretations			
Antimicrobial Resistance Genes			
✓ Detected	KPC (carbapenem-resistance gene)		
⊘ N/A	<i>mecA</i> (methicillin-resistance gene)		
⊘ N/A	<i>vanA/B</i> (vancomycin-resistance genes)		
⚠ NOTE: Antimicrobial resistance can occur via multiple mechanisms. A Not Detected result for the FilmArray antimicrobial resistance gene assays does not indicate antimicrobial susceptibility. Subculturing is required for species identification and susceptibility testing of isolates.			
Gram Positive Bacteria			
Not Detected	<i>Enterococcus</i>		
Not Detected	<i>Listeria monocytogenes</i>		
Not Detected	<i>Staphylococcus</i>		
Not Detected	<i>Staphylococcus aureus</i>		
Not Detected	<i>Streptococcus</i>		
Not Detected	<i>Streptococcus agalactiae</i> (Group B)		
Not Detected	<i>Streptococcus pneumoniae</i>		
Not Detected	<i>Streptococcus pyogenes</i> (Group A)		
Gram Negative Bacteria			
Not Detected	<i>Acinetobacter baumannii</i>		
✓ Detected	<i>Enterobacteriaceae</i>		
Not Detected	<i>Enterobacter cloacae</i> complex		
Not Detected	<i>Escherichia coli</i>		
Not Detected	<i>Klebsiella oxytoca</i>		
✓ Detected	<i>Klebsiella pneumoniae</i>		
Not Detected	<i>Proteus</i>		
Not Detected	<i>Serratia marcescens</i>		
Not Detected	<i>Haemophilus influenzae</i>		
Not Detected	<i>Neisseria meningitidis</i>		
Not Detected	<i>Pseudomonas aeruginosa</i>		
Yeast			
Not Detected	<i>Candida albicans</i>		
Not Detected	<i>Candida glabrata</i>		
Not Detected	<i>Candida krusei</i>		
Not Detected	<i>Candida parapsilosis</i>		
Not Detected	<i>Candida tropicalis</i>		
Run Details			
Pouch:	BCID Panel	Protocol:	BCID
Run Status:	Completed	Operator:	RJones
Serial No.:	00631374	Instrument:	FA2075
Lot No.:	125313		

The purchase of FilmArray System includes a limited, non-transferable license under U.S. Patent No. 5,871,908, owned by Evotec Biosystems GmbH and licensed to Roche Diagnostics GmbH, to use only the enclosed amount of product according to the specified protocols. No right is conveyed, expressly, by implication, or by estoppel, to use any instrument or system under any claim of U.S. Patent No. 5,871,908, other than for the amount of product contained herein.

The purchase of this product includes a limited, nontransferable instrument license under specific claims of one or more U.S. patents as listed on BioFire Diagnostics, Inc.'s Web site (<http://www.biofire.com/LegalNotices/>) (the "Web Site") and owned by the University of Utah Research Foundation and/or BioFire Diagnostics, Inc. Any kits sold with this product and/or discussed herein (i) may be covered by one or more of the U.S. patents, as listed on the Web Site for the product and (ii) include a limited, nontransferable license to use the enclosed amount(s) in such kits according to the specified protocols.